

# Reduced-Voltage RF Shimming for Adiabatic Pulse Design in Parallel Transmission

K. Setsompop<sup>1</sup>, L. L. Wald<sup>2</sup>, and E. Adalsteinsson<sup>1</sup>

<sup>1</sup>EECS, Massachusetts Institute of Technology, Cambridge, MA, United States, <sup>2</sup>A. A. Martinos Center for Biomedical Imaging, MGH, Harvard Medical School, Charlestown, MA, United States

**Introduction:** Adiabatic pulses play an important role in magnetization inversion in the presence of B1 field inhomogeneity. In this work we propose the use of an adiabatic slice selective inversion pulse for parallel RF excitation design. A novel RF shimming algorithm is used to reduce the peak voltage required for the inversion. While the B1 shimming algorithm can be applied in principle to any adiabatic pulse, it is demonstrated here with a hyperbolic secant pulse [1]. Simulation results show that significant reductions in peak voltage and slice inversion non-uniformity can be achieved when compared with traditional RF shimming methods.


**Methods: RF shimming for Adiabatic Inversion:** Conventional RF shimming methods aim to make both the amplitude and phase of the B1 field spatially uniform across the excitation area [2]. This is achieved by applying different amplitude and phase to the RF pulses of each excitation coils. Mathematically, this problem can be stated as:  $\min_b \sum_{x,y} \|B_1(b, x, y) - B_{1MEAN}(b)\|_2$ , where  $b$  is the complex vector of voltages applied to

the coils,  $B_1(b, x, y)$  is the resultant B1 field after shimming, and  $B_{1MEAN}$  is the average field across the profile. To achieve uniformity, cancellation of the B1 fields produced by the excitation coils is needed; suggesting increased RF amplitudes are required. Using an adiabatic RF pulse to create uniform inversion places no restriction on the uniformity of the amplitude and phase of the B1 field. It is only required that the B1 field across the volume be above a certain threshold. It can be seen that the conventional RF shimming is more restrictive than what is required for adiabatic inversion. To reduce SAR, it is desirable to achieve the inversion at the lowest voltage which satisfies the adiabaticity conditions. With this in mind, we propose the following optimization algorithm to calculate the complex ratio of the voltages used in RF shimming of adiabatic pulses:


$\max_b \left\{ \min_{x,y} |B_1(b, x, y)| \right\}$  such that  $|b| \leq 1$ . We seek to maximize the minimum B1 field for

the case where all the voltages applied to the coils are restricted to be less than a cutoff amplitude (normalized to one here). Once this optimization has been carried out, to perform the inversion, the resulting voltages are scaled up so that the minimum B1 field after shimming is above the threshold required for adiabaticity. **Bloch Simulation:** Performance of the traditional and the new algorithms for RF shimming are compared in the case of adiabatic inversion using an 8-channel loop coil array used previously for parallel excitation [2]. The well-known hyperbolic secant slice selective inversion pulse is used, with slice thickness of 0.5 cm, TBW of 10, and pulse duration of 9 ms.

**Results and discussion:** Fig1. shows the simulated result of the adiabatic inversion at various B1 field amplitudes, and values of corresponding adiabatic factor (k). It can be seen that the hyperbolic secant pulse creates a uniform slice selective inversion when the B1 amplitude is above a certain threshold (around k = 3), and is relatively insensitive to increases in RF amplitude over this threshold performing well up to around k = 8. Fig2. shows the B1 field distribution after the RF shimming algorithms have been applied. The 8-channel coil array used for parallel excitation is not particularly suited for RF shimming. Large central dips can be observed (top row) when the traditional shimming is used. Also shown (center row) is a relaxed traditional shimming where the uniformity has been traded off for reduced voltage by cutting off low eigenvalues in an SVD-based inversion. Shown in the bottom row is the resulting profile when the new shimming algorithm is used. Although the phase is less uniform, this is unimportant for the adiabatic pulse. On the other hand, the resulting B1 magnitude is much more uniform (B1max/B1min ratio are 3.5, 3.3, and 2.1 for the three

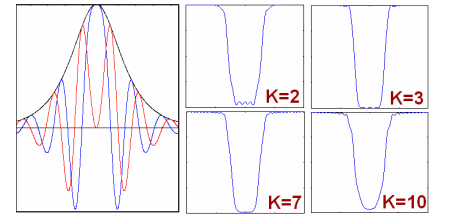

**Fig1. Hyperbolic secant pulse (left), and the resulting slice selective inversion at various adiabatic factors (right)**

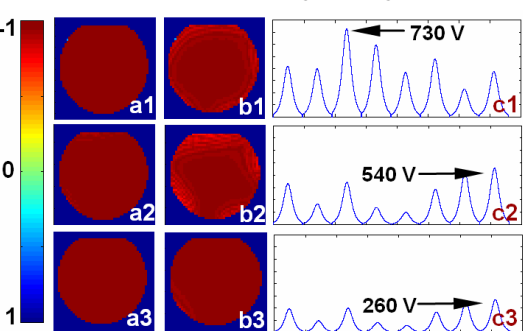


**Fig3. Inversion profile at z = 0 (left), z = 0.15 cm (center), and the concatenated magnitude of the adiabatic pulse used on the 8 coils (right); for traditional shimming (top row), relaxed traditional shimming (center row), and new shimming (bottom row)**

ratio of B1max/B1min in the traditional and the relaxed traditional methods cause the adiabatic factor (k) in region of high B1 field to be very high (>8), causing suboptimal slice selection in this region as seen in Fig 3 (b1&b2 at z = 0.15 cm). On the other hand, this ratio is small in the new shim method, resulting in very uniform profile. We also note that the peak voltage reduction is dramatic, from 730V to 260V for the proposed vs. traditional RF shimming. **Conclusion:** A novel RF shimming algorithm has been proposed and evaluated for an 8-channel loop array for the design of adiabatic inversion for parallel excitation. Simulation results show a significant reduction in peak voltage and improved slice inversion uniformity when compared with traditional RF shimming methods.

**Acknowledgements:** Siemens Medical Solutions, NIH P41RR14075, R. J. Shillman Career Development Award.

**References:** 1. Silver M.S., Joseph R.I., Hoult D.I., JMR 1984;59:347 2. Setsompop K. et al, MRM 2006;56:1163.

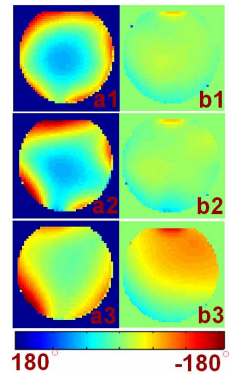

**Fig2. Magnitude (left) and phase (right) after traditional RF shimming (top), relaxed traditional shimming (center), and new shimming (bottom).**